



REPLACEMENT SHEET

Fig. 1A
(PRIOR ART)

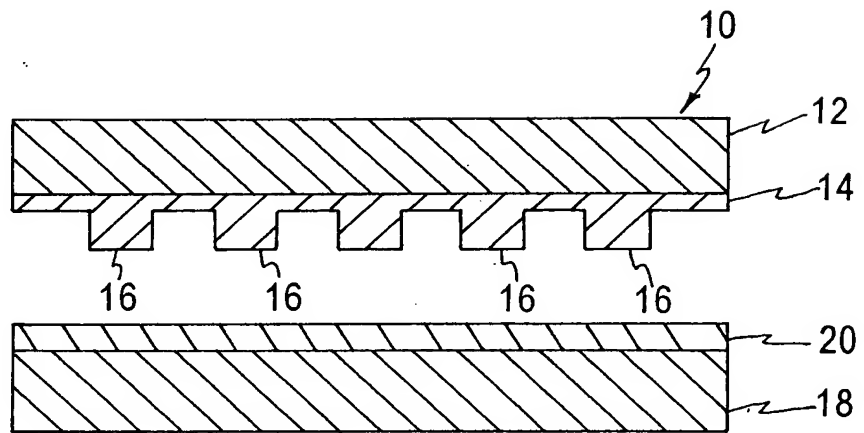


Fig. 1B
(PRIOR ART)

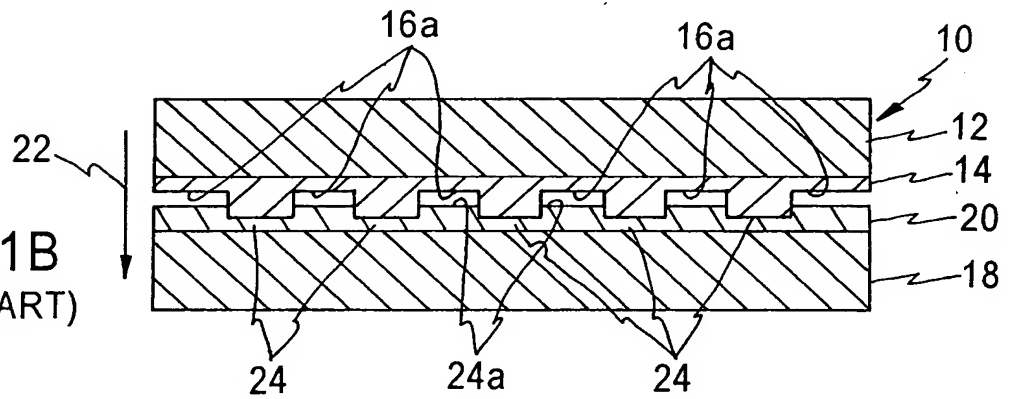


Fig. 1C
(PRIOR ART)


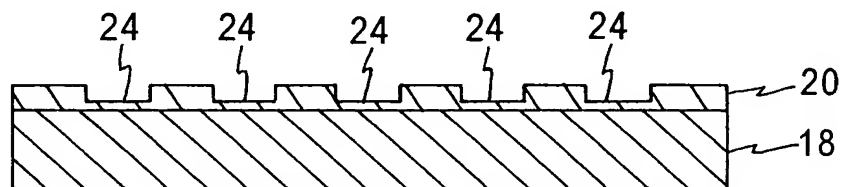


Fig. 1D
(PRIOR ART)



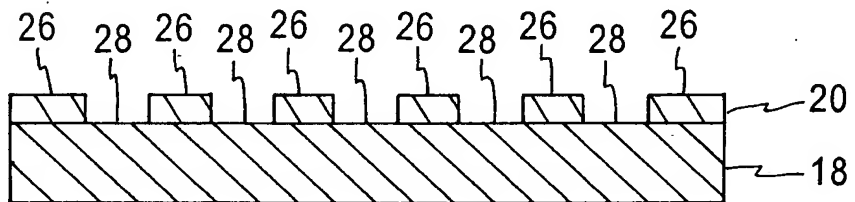

REPLACEMENT SHEET

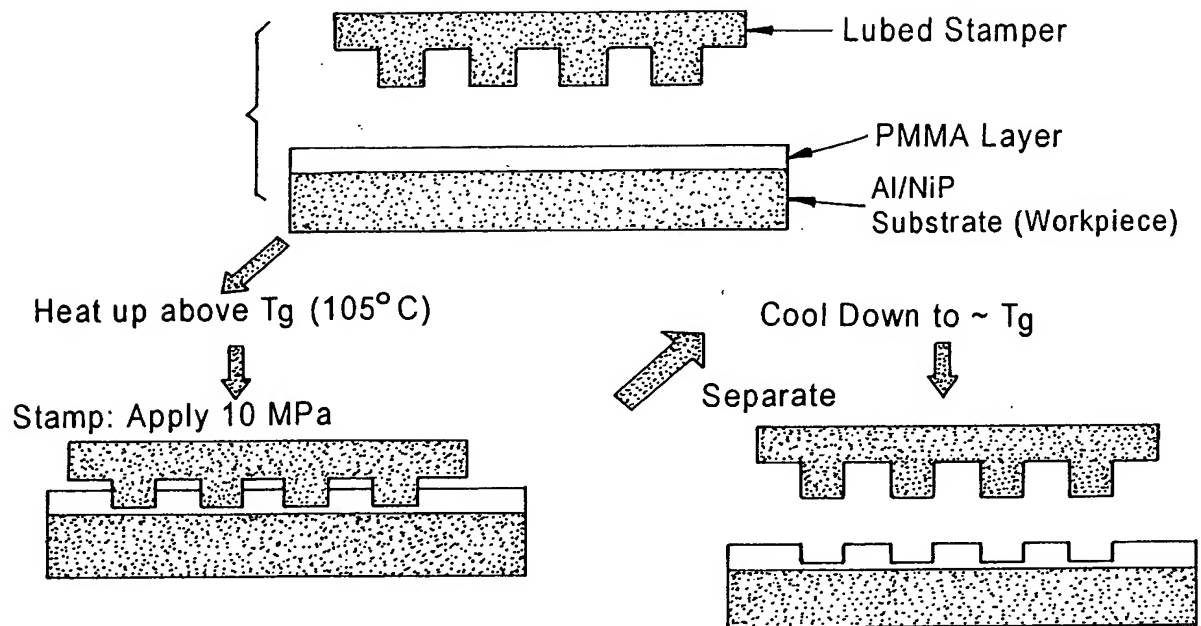


Fig. 2 (PRIOR ART)

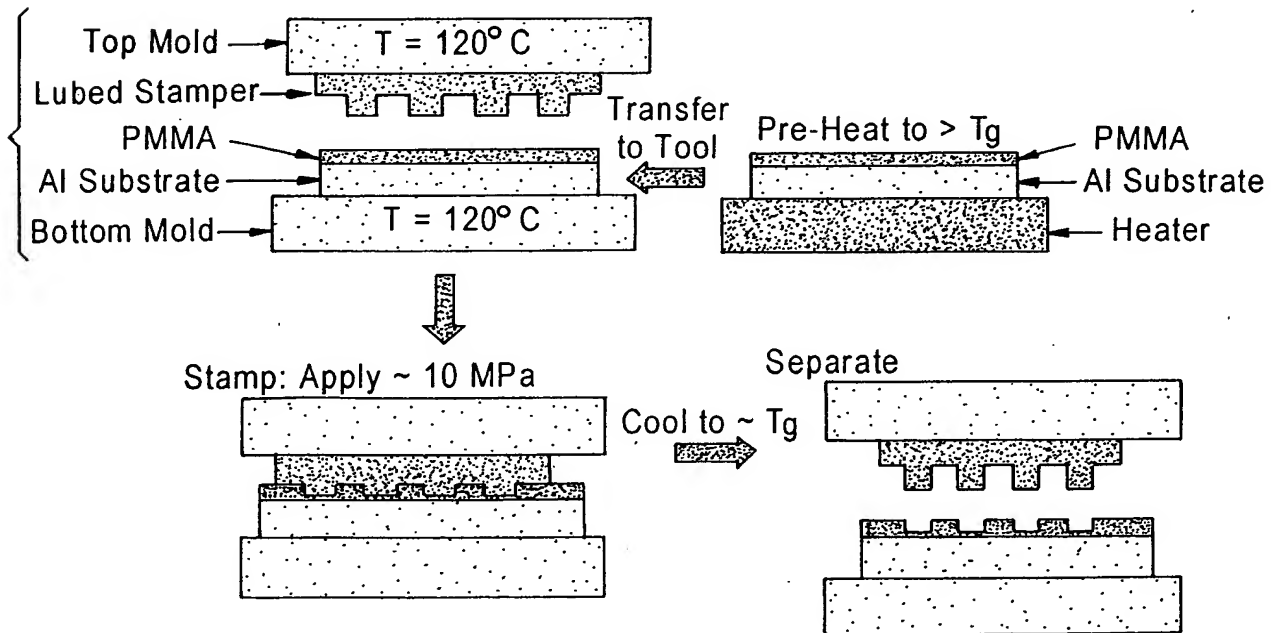


Fig. 3



REPLACEMENT SHEET

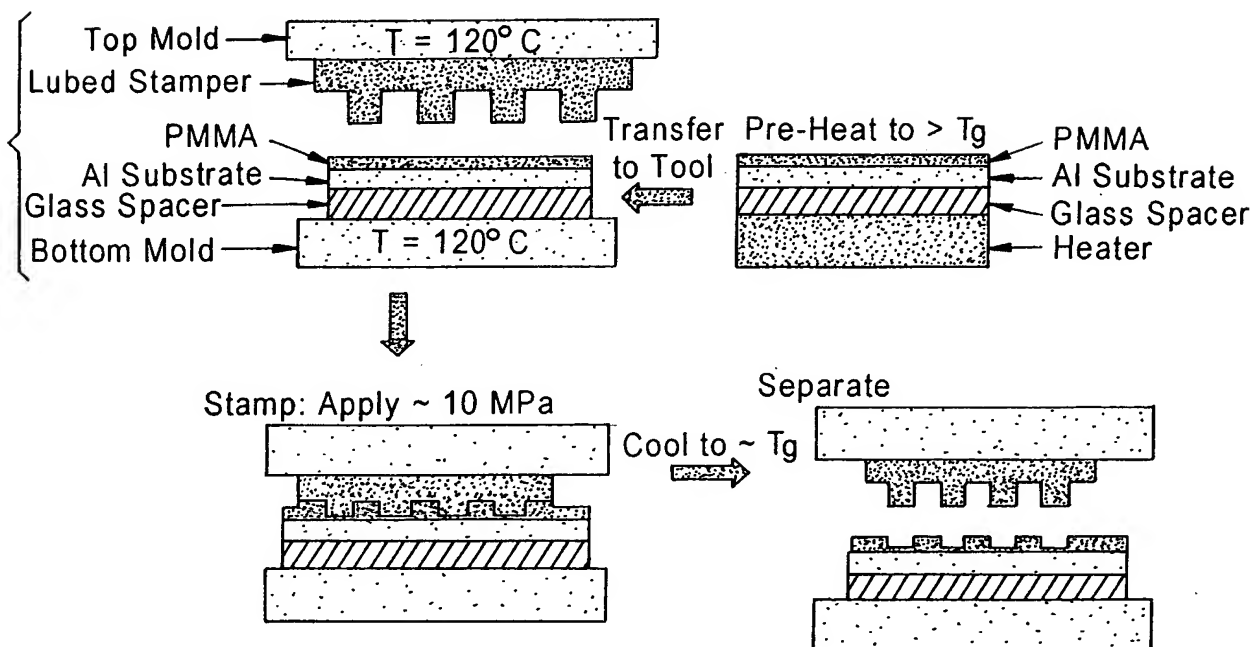


Fig. 4

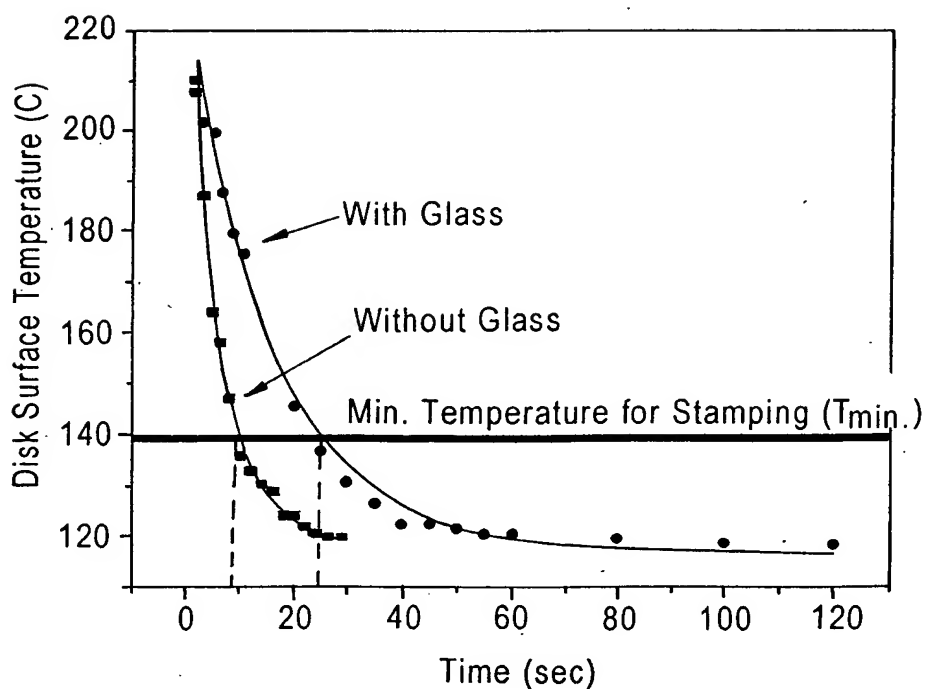


Fig. 5



REPLACEMENT SHEET

Digital Instruments	ManoScope
Scan Size	5.020 μM
Scan Rate	1.969 Hz
Number of Samples	512
Image Data	Height
Data Scale	400.0 nM

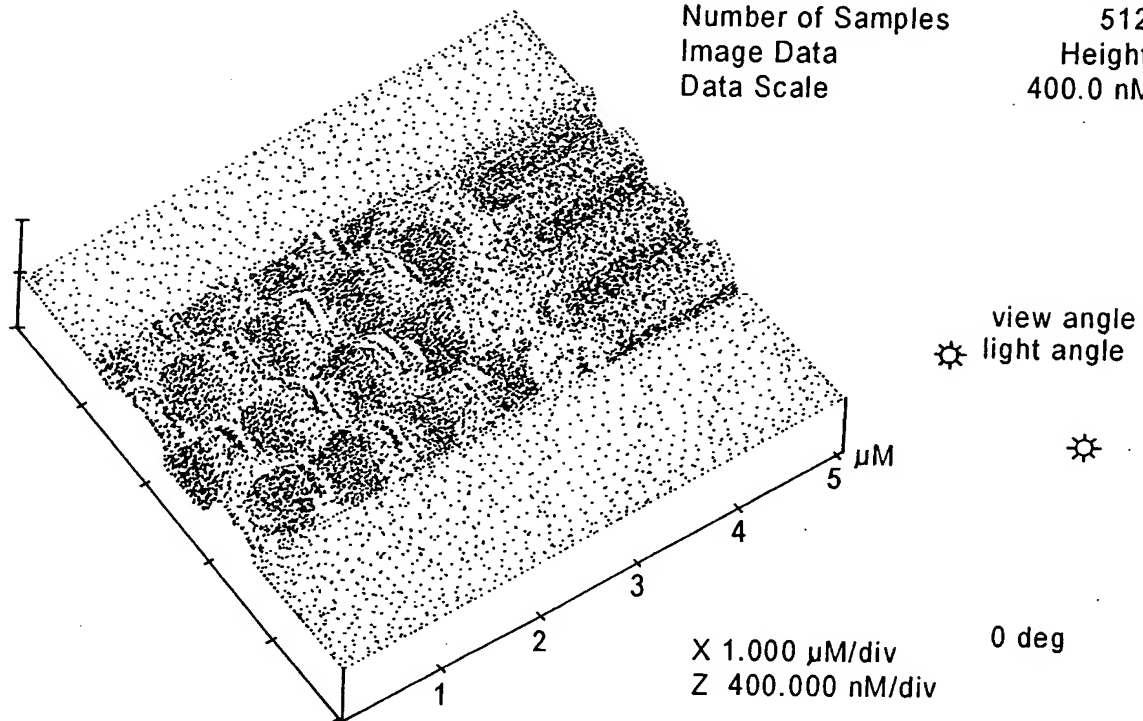


Fig. 6